

FIG. 1A

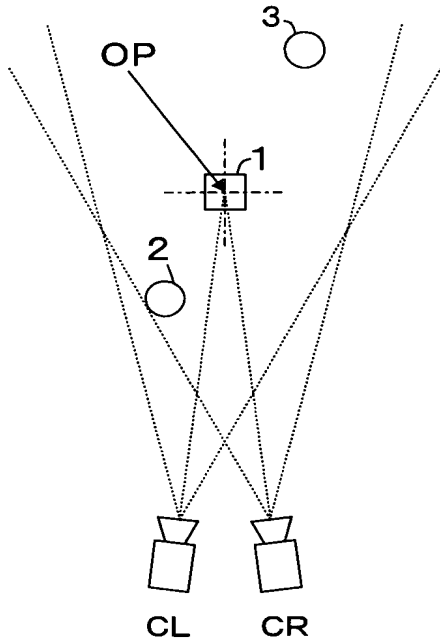


FIG. 1B

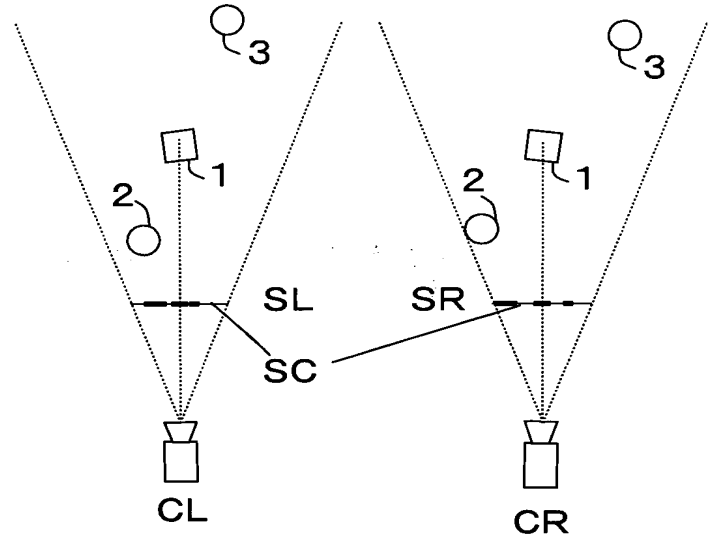


FIG. 1C

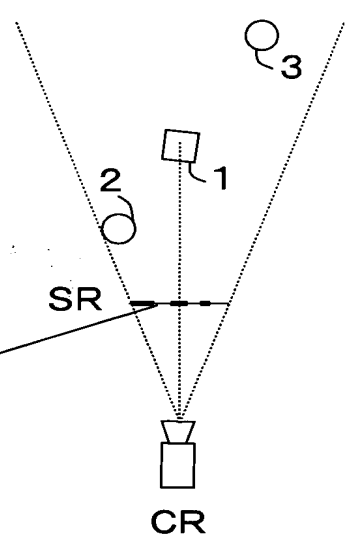


FIG. 1D

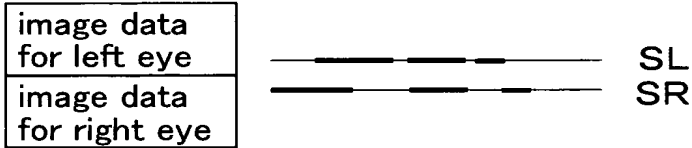


FIG. 1E

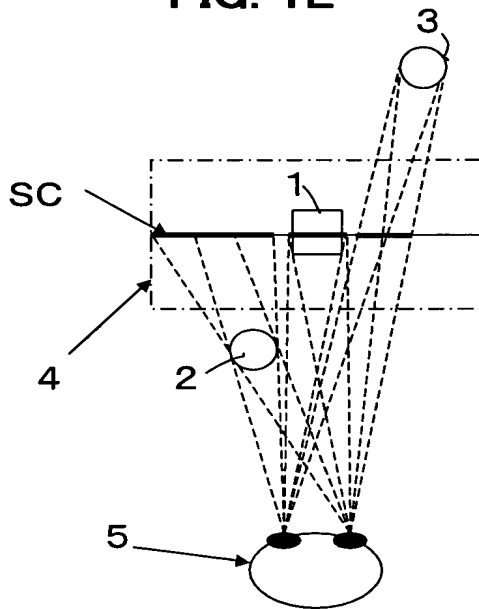


FIG. 1F

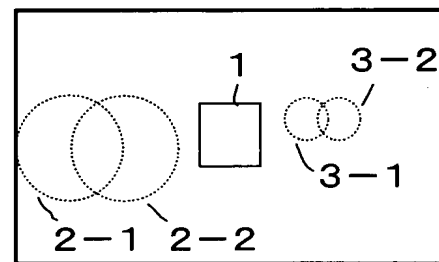


FIG. 2

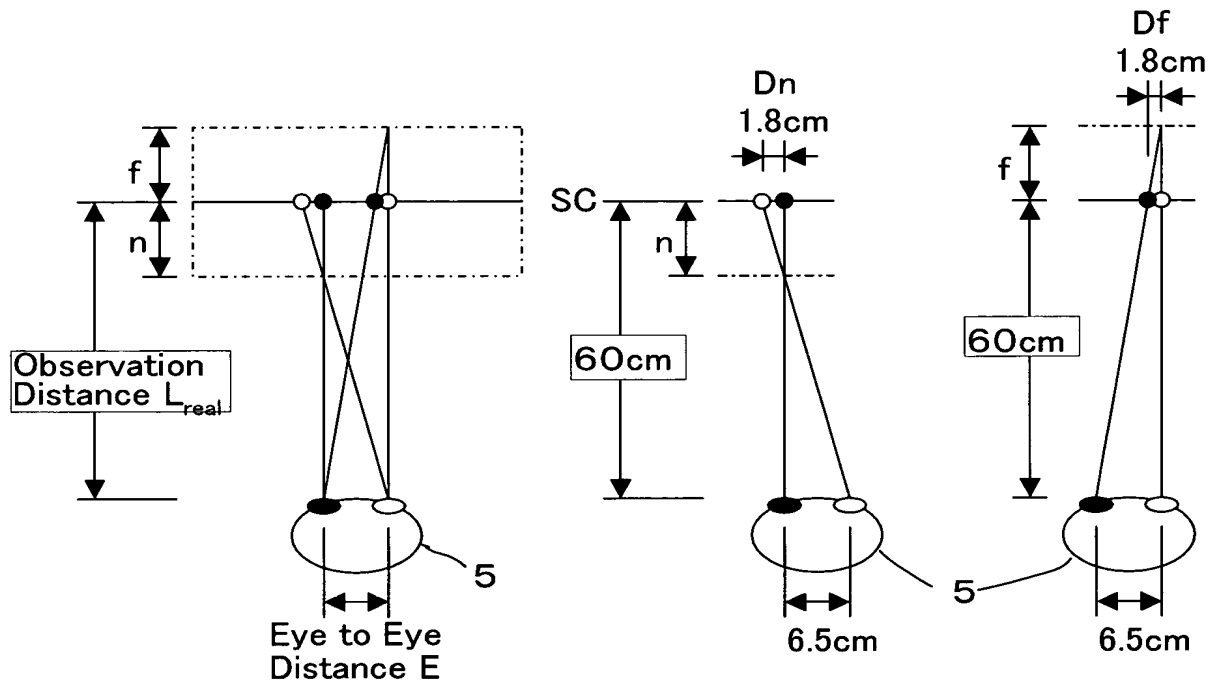


FIG. 3A

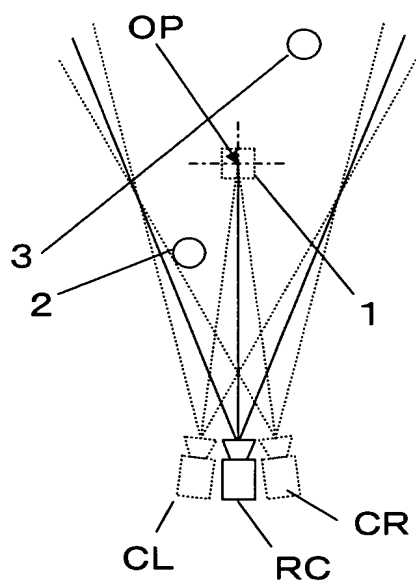


FIG. 3B

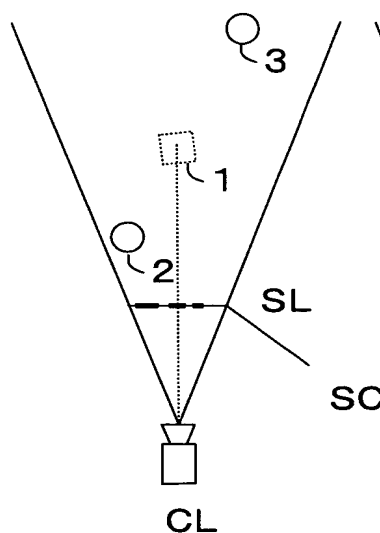


FIG. 3C

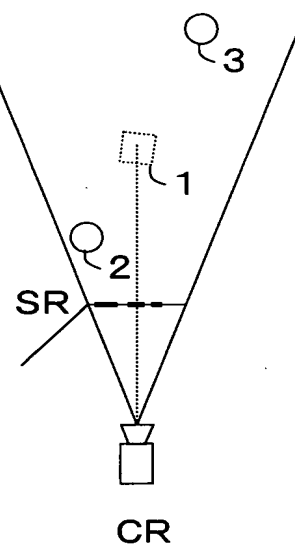


FIG. 3D



FIG. 3E

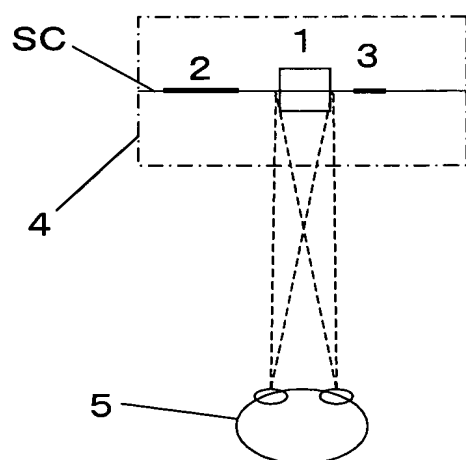


FIG. 3F

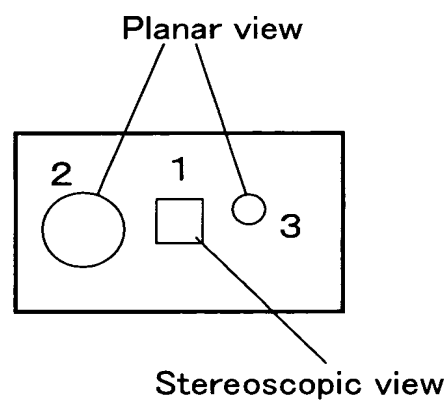


FIG. 4A

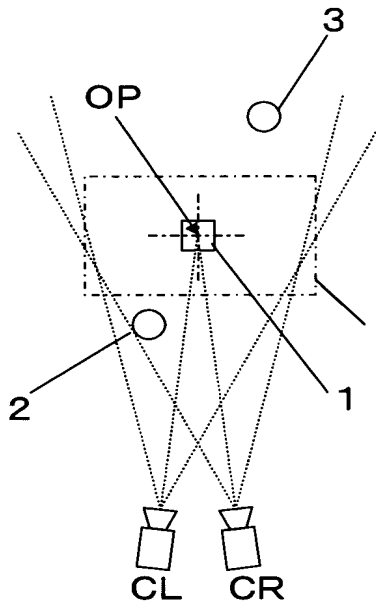


FIG. 4B

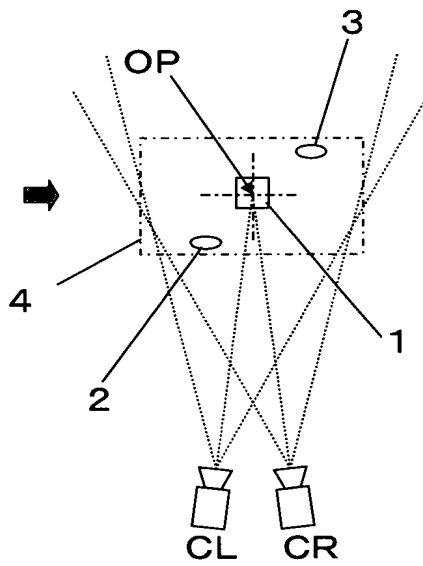


FIG. 4C

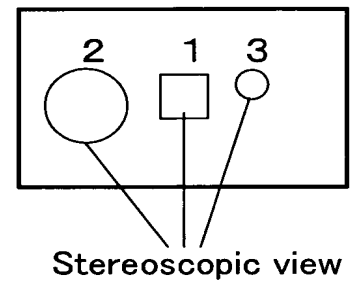


FIG. 5A

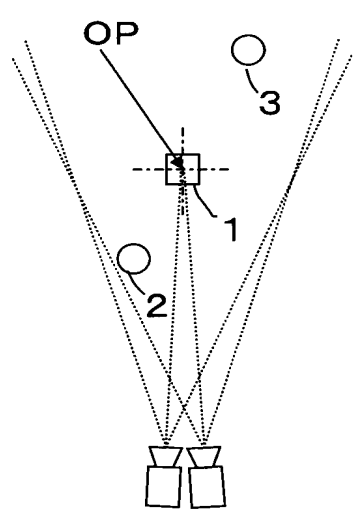


FIG. 5B

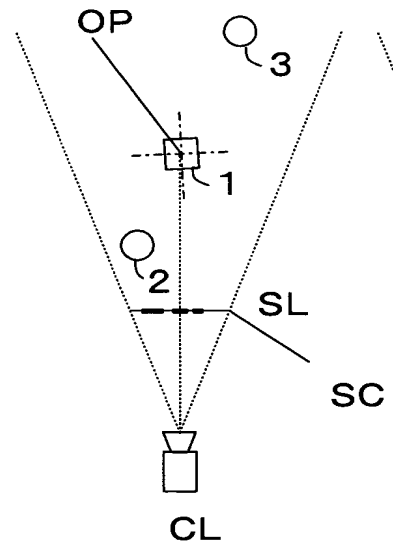


FIG. 5C

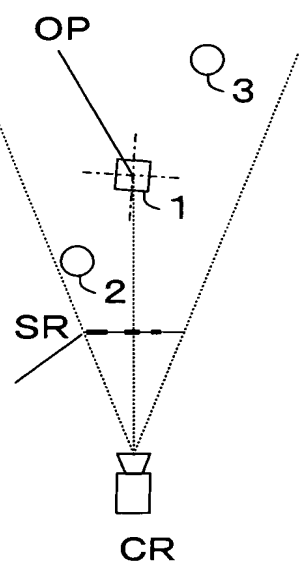


FIG. 5D

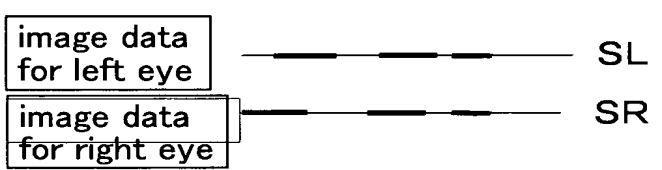


FIG. 5E

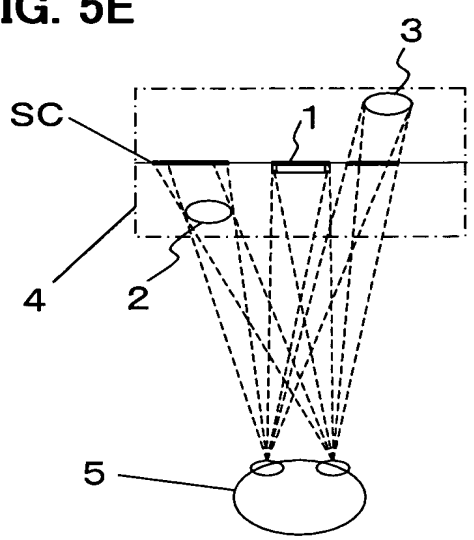


FIG. 5F

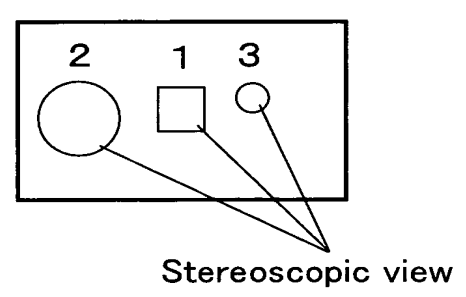


FIG. 6A

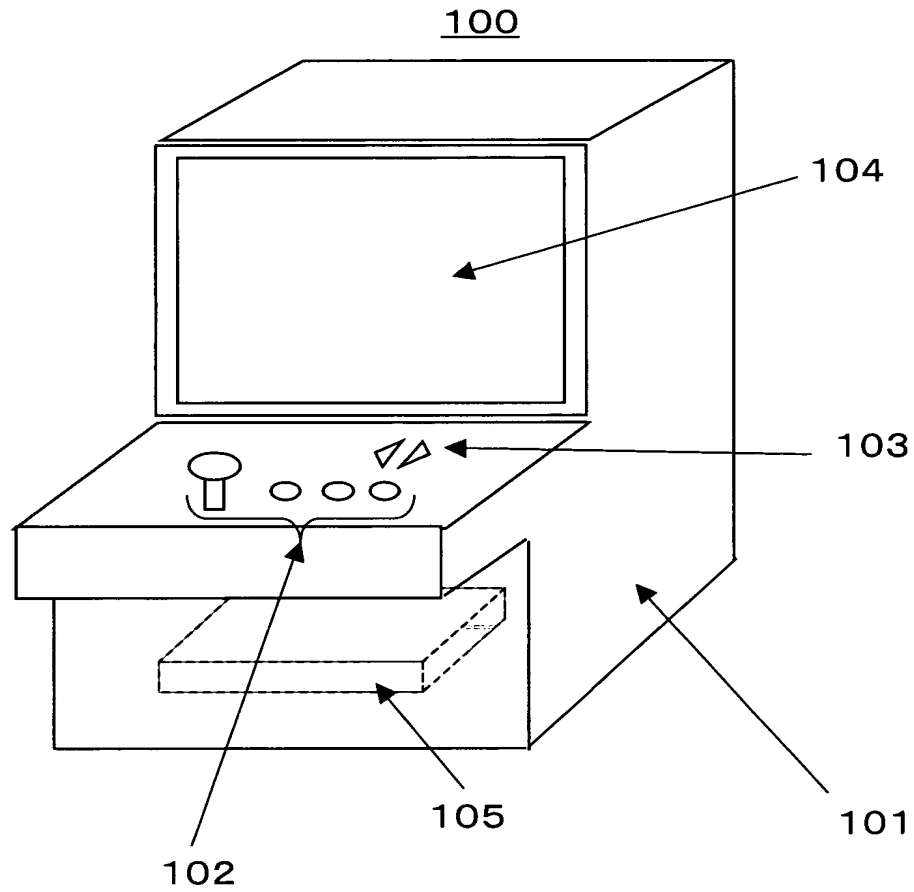


FIG. 6B

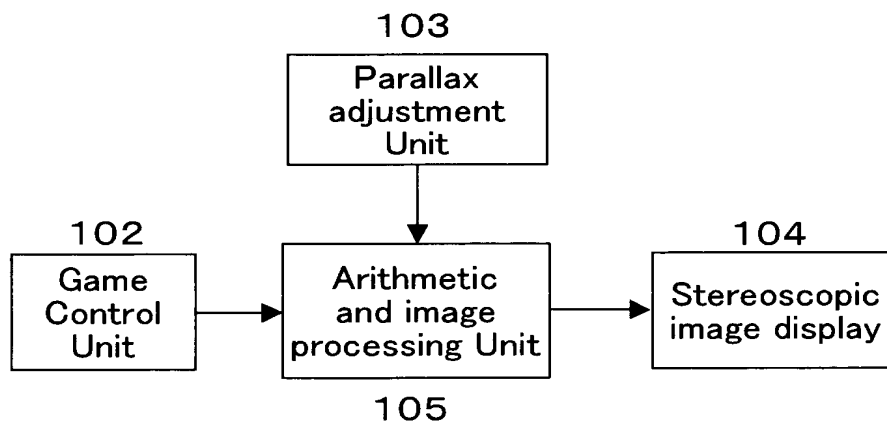


FIG. 7

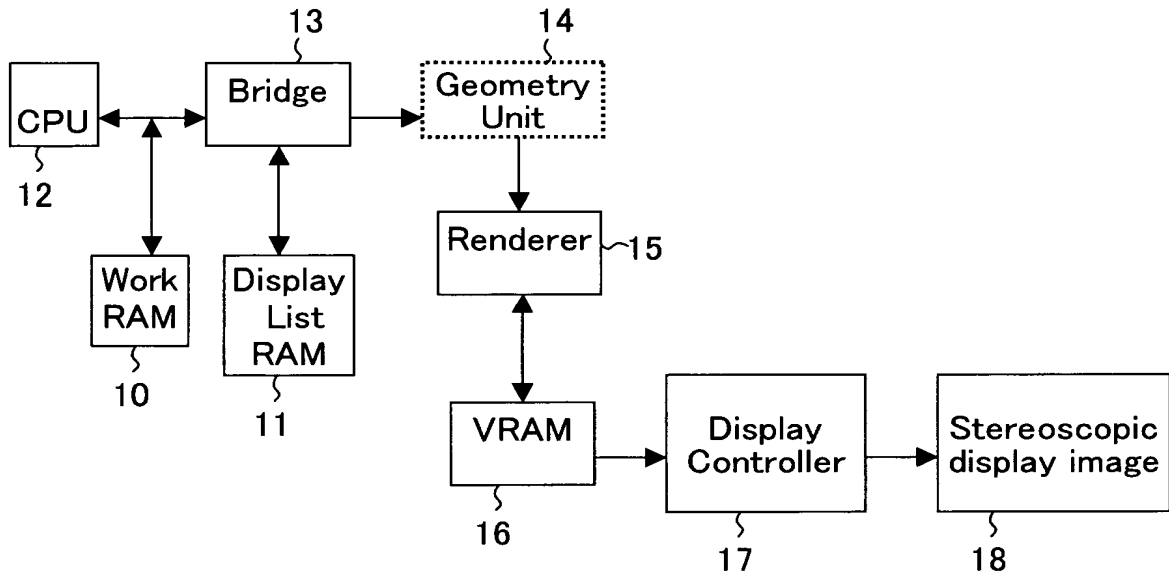


FIG. 8

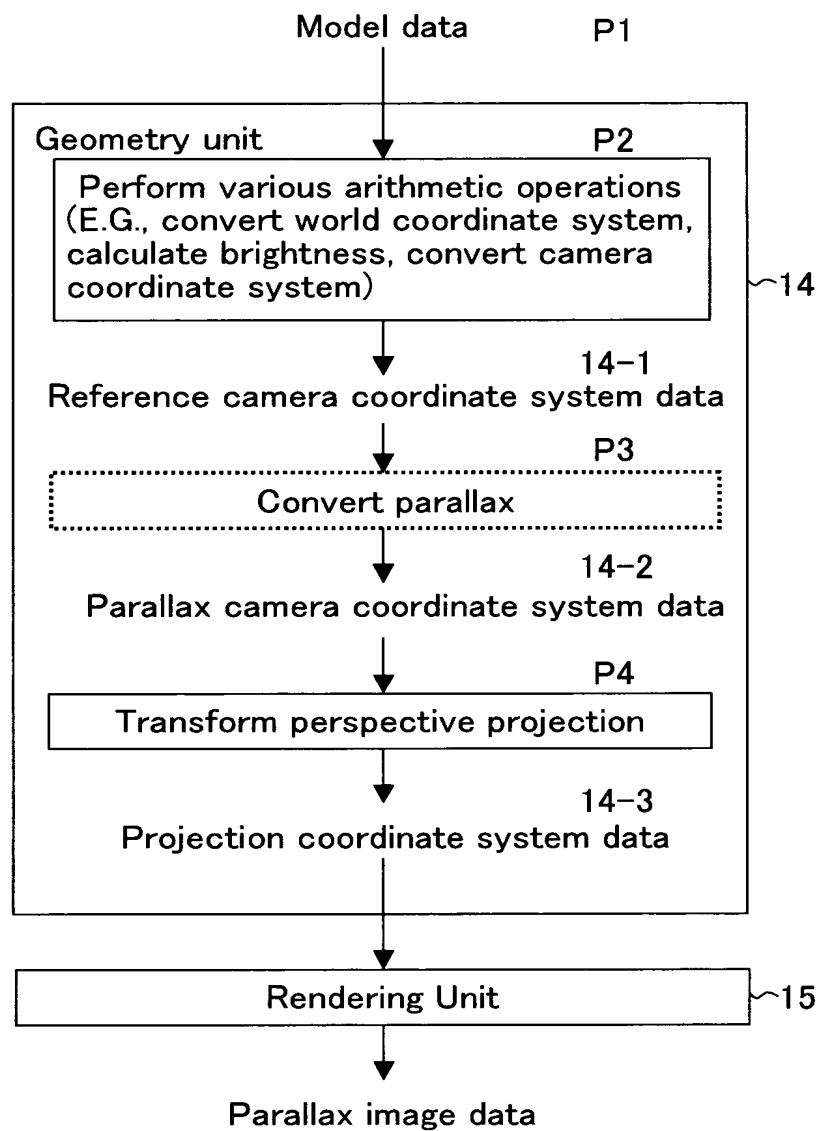


FIG. 9A

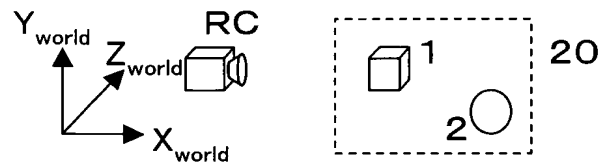


FIG. 9B

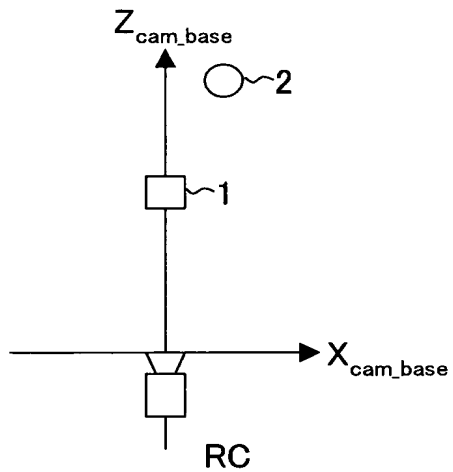


FIG. 9C

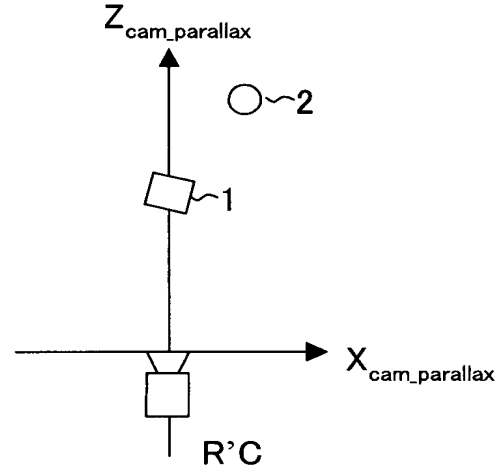


FIG. 9D

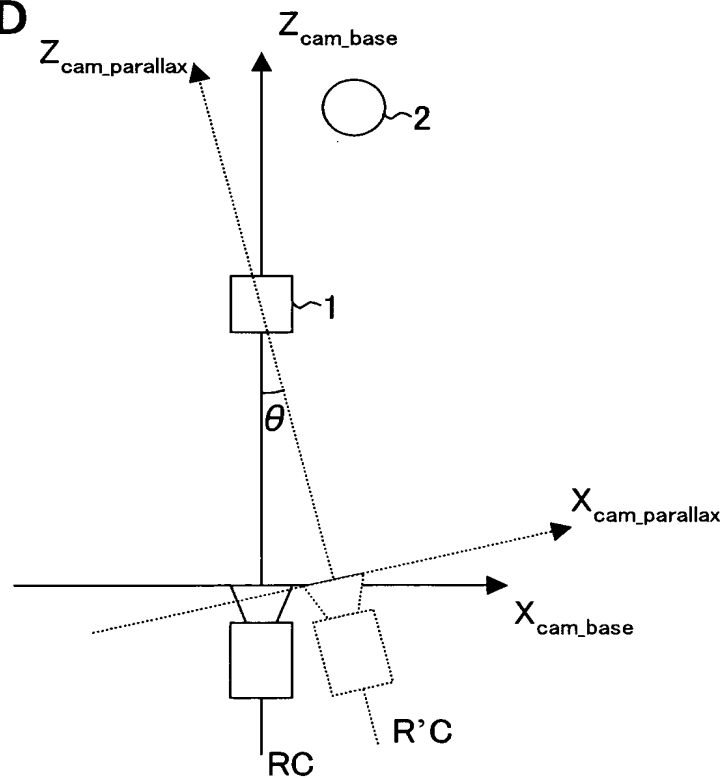


FIG. 10A

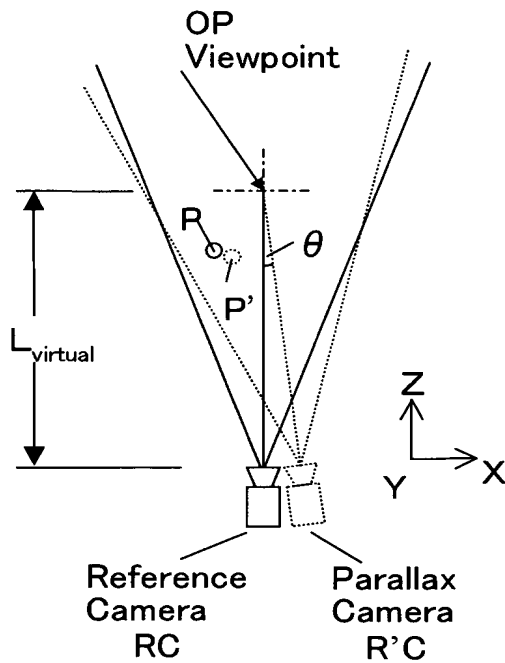


FIG. 10B

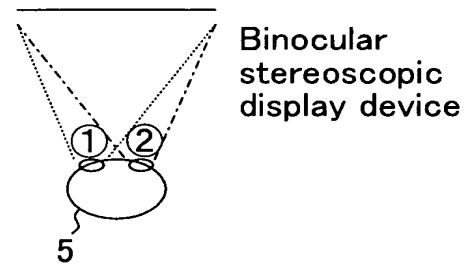


FIG. 10C

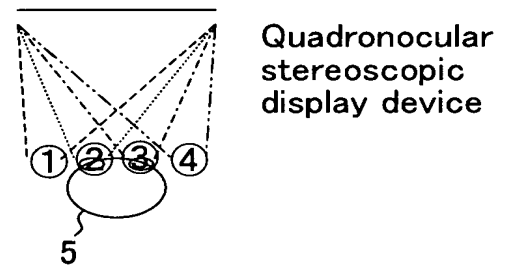


FIG. 11

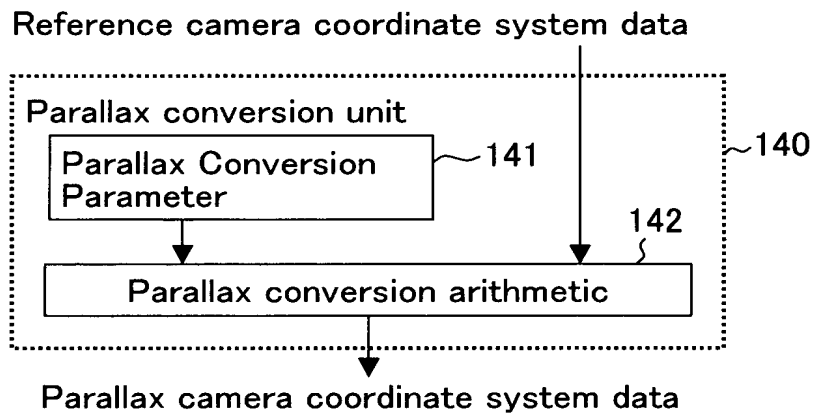


FIG. 12

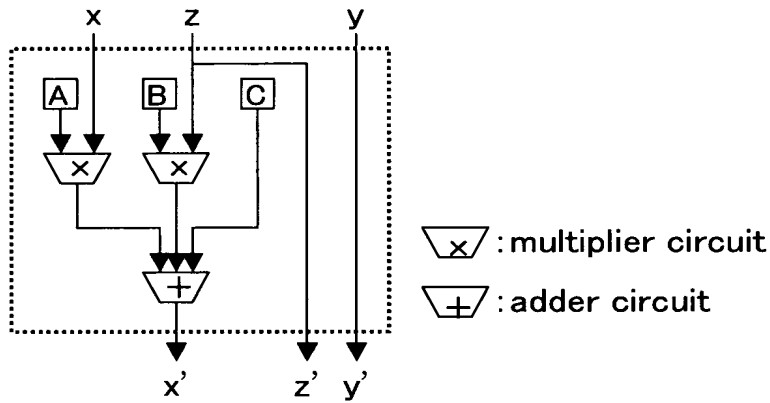
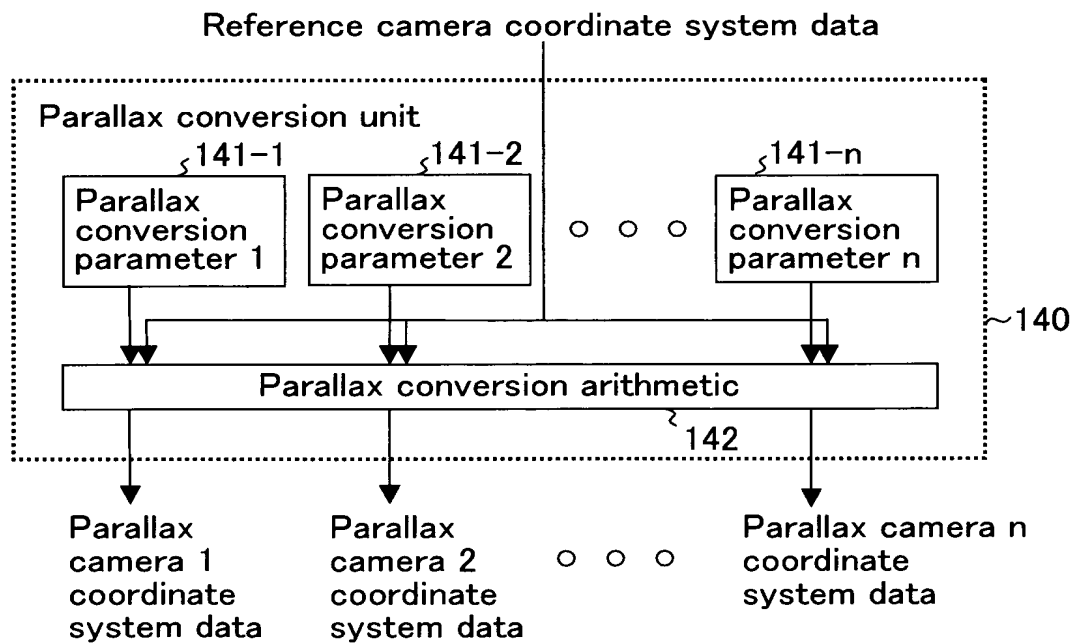


FIG. 13



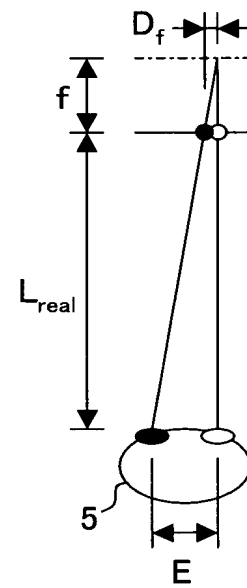


FIG. 15A

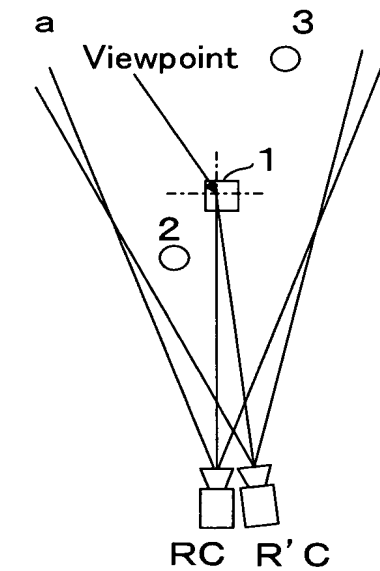


FIG. 15B

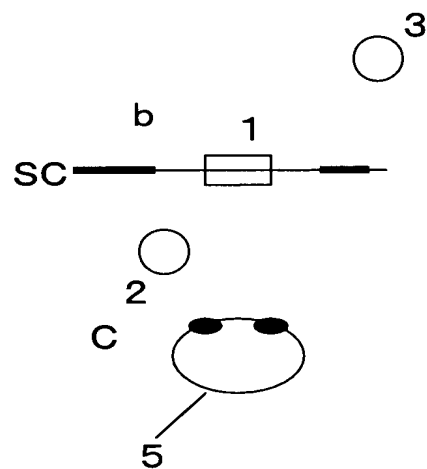
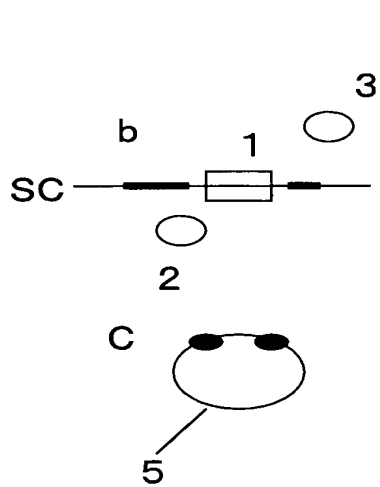

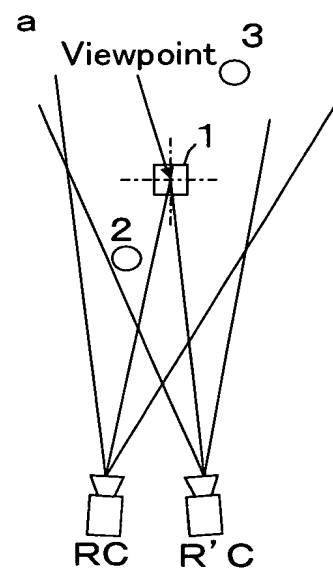


FIG. 16

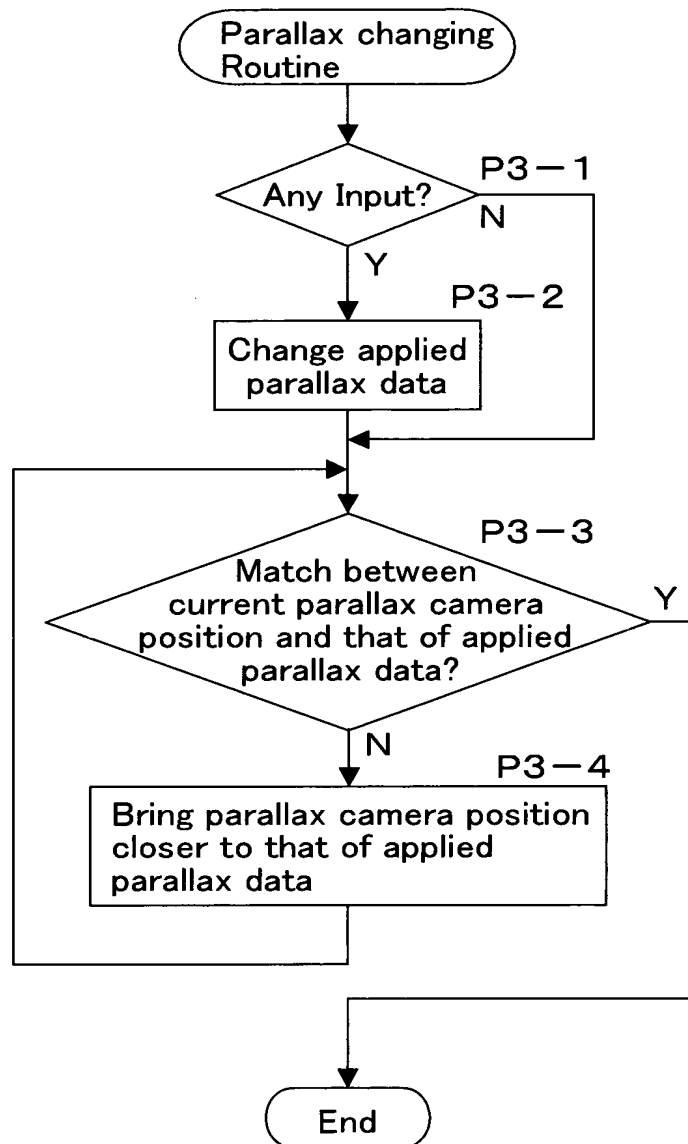


FIG. 17

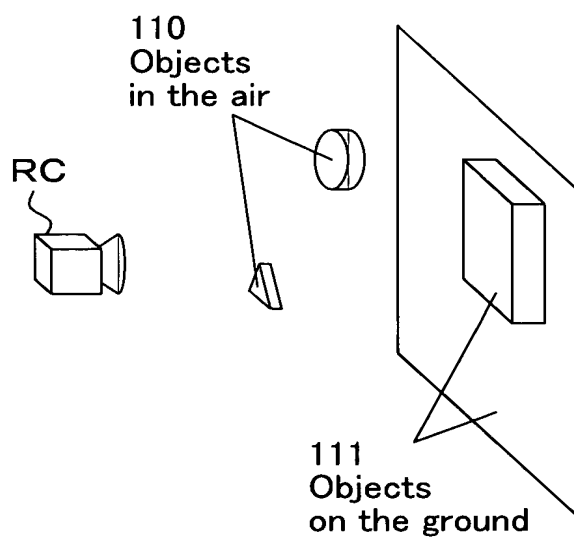


FIG. 18

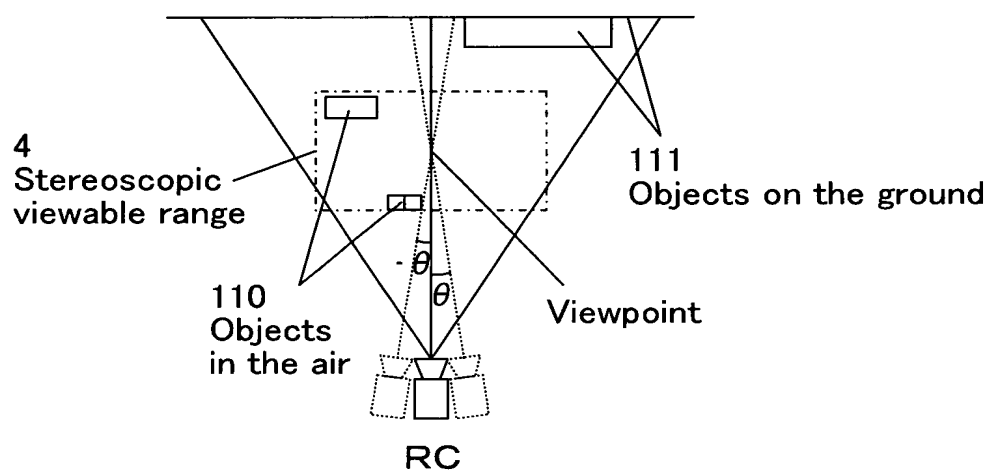


FIG. 19

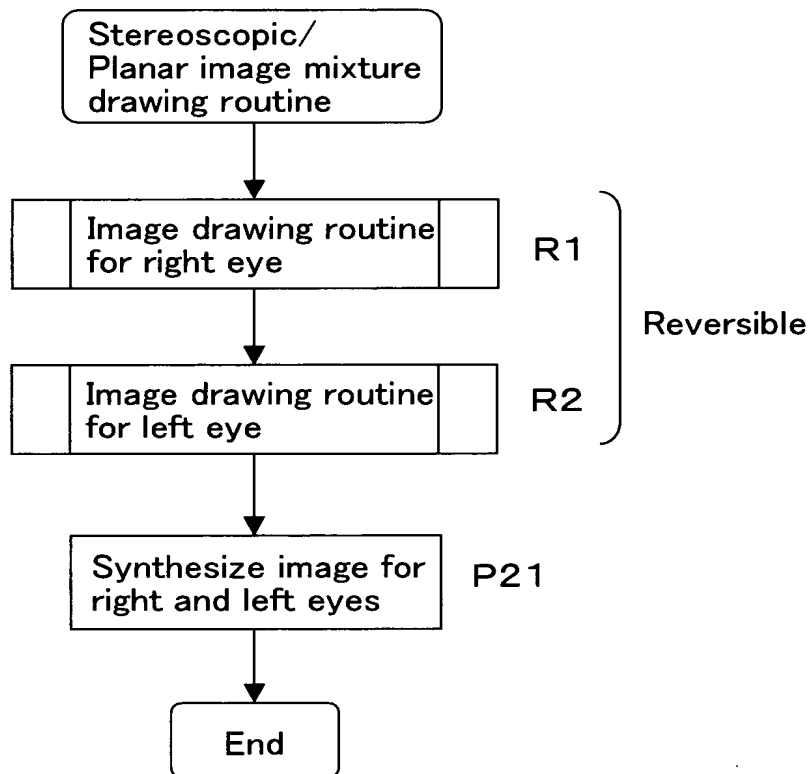


FIG. 20

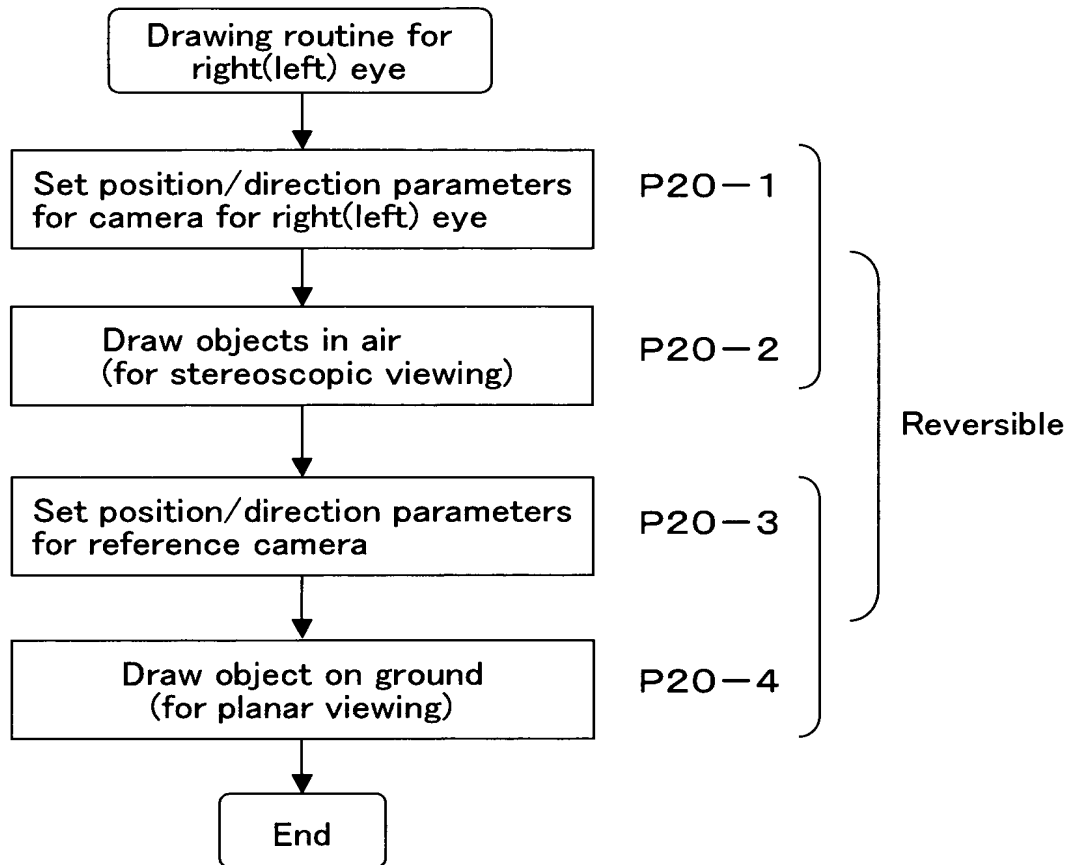


FIG. 21A

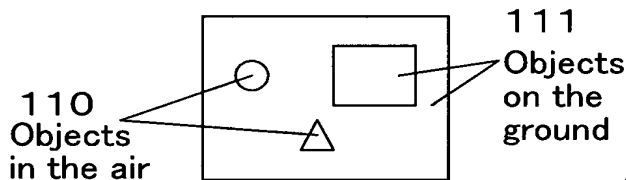


FIG. 21C

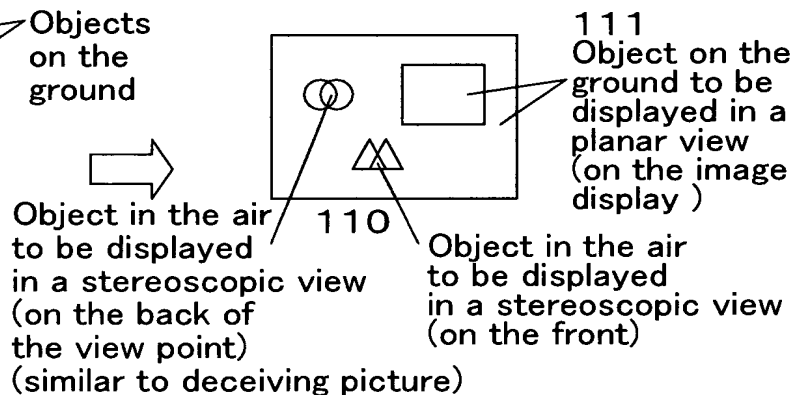


FIG. 21B



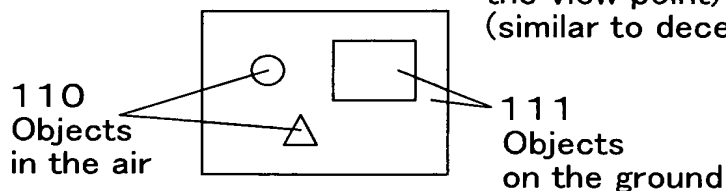


FIG. 22A

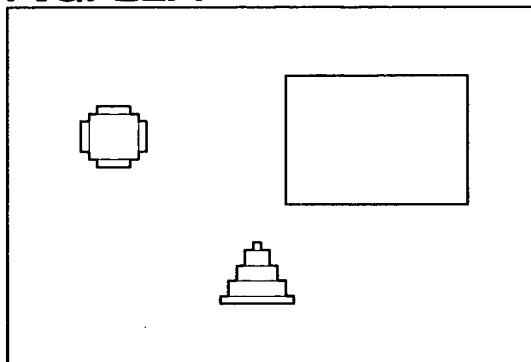


drawn image for left eye

FIG. 22B

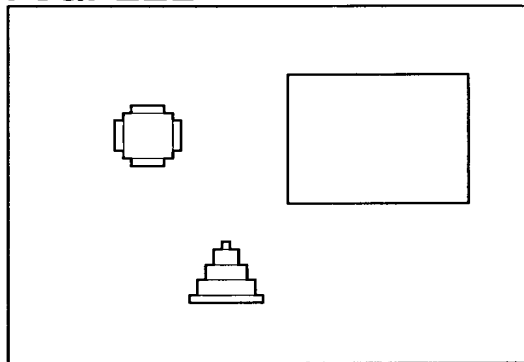


drawn image for right eye

FIG. 22C

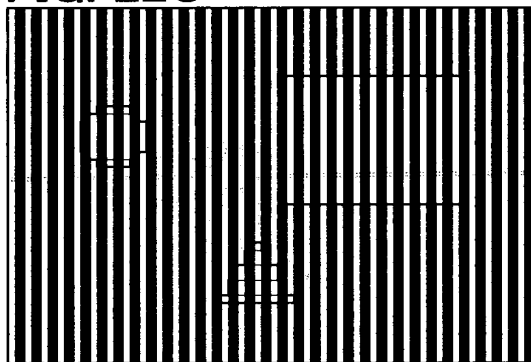


extraction image for left eye

FIG. 22D

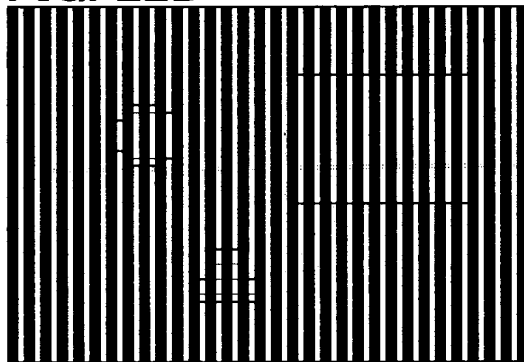

extraction image for right eye

FIG. 22E

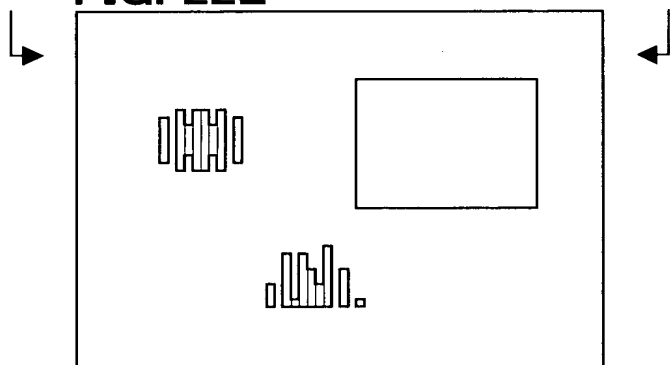

synthesized image for stereoscopic viewing